




# CoperniFUS: A flexible Python-based GUI for stereotaxic Focused UltraSound (FUS) experiment planning

Tom Aubier <sup>1</sup>, Ivan M. Suarez-Castellanos <sup>1</sup>, and W. Apoutou N'Djin <sup>1</sup>

<sup>1</sup> LabTAU, INSERM, Centre Léon Bérard, Université Claude Bernard Lyon 1, F-69003, Lyon, France   
Corresponding author

DOI: [10.21105/joss.08128](https://doi.org/10.21105/joss.08128)

## Software

- [Review](#) 
- [Repository](#) 
- [Archive](#) 

Editor: [Kevin M. Moerman](#)  

## Reviewers:

- [@richardkoehler](#)
- [@Julie-Fabre](#)
- [@plooney](#)

Submitted: 07 February 2025

Published: 24 July 2025

## License

Authors of papers retain copyright and release the work under a Creative Commons Attribution 4.0 International License ([CC BY 4.0](#)).

## Summary

Focused Ultrasound (FUS) is gaining increasing interest for its potential as a minimally invasive and precisely targeted alternative to conventional neurostimulation techniques. Although reversible changes in the activity of neural structures have been reported as far back as 1929 (Harvey, 1929), comprehensive descriptions of the short- and long-term effects of ultrasound on neural structures are still lacking to achieve neurostimulation with satisfactory levels of control and safety. Delivering well-characterized FUS pulses with a high degree of spatial selectivity, along with local assessment of the state and activity of specific brain regions, is crucial in pursuing this research. Unlike most electrophysiology procedures involving compact needle-like probes that can be achieved using a stereotaxic frame limited to three degrees of freedom, FUS experiments on small *in vivo* models often require the implementation of complex probe layouts to assess the activity of the stimulated neural structures. Treatment planning, evaluation of acoustic parameters through simulations, and post-processing of results often rely on distinct software programs with their own coordinate systems, which greatly complicates the integration, analysis, and interpretation of key information—thus limiting the ability to properly describe the spatiotemporal aspects of FUS neurostimulation dynamics.

Designed around a unified coordinate system architecture, CoperniFUS is built to address this challenge by offering a versatile software platform for planning stereotaxic FUS procedures. Moreover CoperniFUS provides the possibility to take anatomical variability into consideration by including the registration of anatomical landmark.

## Statement of need

In an effort to assess the therapeutic potential of ultrasound neurostimulation, studies have sought to characterize the effect of ultrasound on the biochemical microenvironment of brain structures after stimulation. While tools like Magnetic Resonance Spectroscopy (MRS) offer a non-invasive way of assessing the concentrations of metabolites *in vivo*, they come with significant limitations. Concentration measurements are non-specific, only representative of the total metabolic, extra- and intracellular quantity of a compound (Dyke et al., 2017). The spatial selectivity of the method is also limited to minimum voxel volumes of several  $cm^3$ . Finally, the difficulties arising from the integration of FUS transducers in MRIs are preventing the further investigation of *online* effects (Yaakub et al., 2023).

Studies on rodent models have been pursued using invasive methods such as microdialysis (Min et al., 2011; Yang et al., 2012). Although these studies report effects of FUS stimulations on dopamine, serotonin or GABA levels, their observations are restricted to low ultrasound central


frequencies resulting in poorly spatially selective stimulations, hindering accurate evaluation of region-specific responses. Despite the interest in characterizing spatially selective stimulations to characterize any region-dependence (Murphy et al., 2024; Suarez-Castellanos et al., 2021), the choice of low frequencies is typically made to maximize energy transfer through the skull and minimize pressure field distortions. Transducer placement and targeting of the structure is empirical, based on trigonometric evaluation of the focus relative to reference atlases.

With the growing interest in transcranial ultrasound therapeutic approaches, extensive research has been conducted to develop and validate computational models of acoustic wave propagation through the skull. Although a number of tools and formalisms exist (J.-F. Aubry et al., 2022; Murphy et al., 2025), *k-Wave* (Treeby & Cox, 2010) has been widely adopted in the field of ultrasound neurostimulation specifically (Constans et al., 2018; Verhagen et al., 2019; Yaakub et al., 2023). Acoustic simulations in this context are performed using standalone Matlab scripts for the definition of acoustic sources and domains. Acoustic domains are defined either directly based on CT or pseudo-CT scans (J.-F. Aubry et al., 2003), or by constructing maps from rasterized brain and skull meshes. Registration of the transducer location relative to targeted brain structures is often achieved using frameless optical tracking neuronavigation systems on human or non-human primate subjects (Murphy et al., 2025; Pichardo, 2023; Sammartino et al., 2020). However, empirical methods are usually chosen in small rodent experiments due to the space constraints associated with these models.

Targeting of brain structures is achieved using reference atlases registered to MRI scans of subjects when available. However for small animals, these images are typically not acquired in a systematic way. Targeted structures coordinates are thus directly evaluated on reference atlases, based on an anatomical landmark such as the Bregma skull suture on rats and mice (Kleven et al., 2023; Wang et al., 2020). Morphological variability between subjects can compromise experiments if it is not taken into account, however registration of reference atlases to anatomical measurements can be tedious and is rarely reported in rodent studies.

## Features

In this context we developed CoperniFUS, a modular software tool offering a common coordinate manipulation platform specifically suited for stereotaxic experiments. Currently available modules allow the manipulation of brain atlases, meshes. They also enable *in situ* *k-Wave* acoustic simulations, with the aim of facilitating the coupling of FUS neurostimulation setups with standard electrophysiology methods such as microdialysis (Min et al., 2011), fiber photometry (Murphy et al., 2024) or fast-scan cyclic voltammetry (Olaitan et al., 2024). With the emergence of Python as the programming language of choice in neuroscience (Muller et al., 2015), we chose to design a Python tool that can be easily tweaked and augmented with specialized modules to address a large range of research needs involving stereotaxic frame-based experiments.

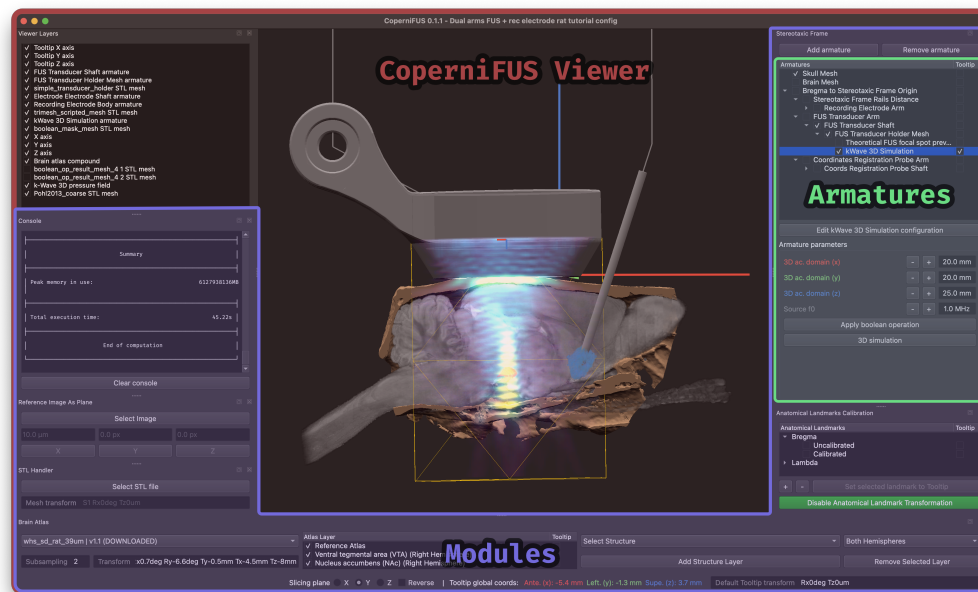


**Figure 1:** Overview of CoperniFUS's Graphical User Interface architecture.

As of the writing of this article, CoperniFUS 0.1.2 currently enables: 1. Facilitated stereotaxic targeting of specific brain structures for a large range of species thanks to the integration of the BrainGlobe API (Claudi et al., 2020). 2. Arbitrary stereotaxic frames can be constructed using a flexible dictionary-based editor. Discrete stereotaxic frame elements (referred as Armatures) can be associated in a hierarchical tree structure, allowing operations such as mesh boolean operations or acoustic simulations to be performed in any coordinate reference frame. 3. In the absence of whole head CT or MRI scans that allow for accurate atlas registration, CoperniFUS provides a means of minimizing the targeting errors that can arise from anatomical variability. To that end, 3D objects such as atlases or skull meshes can inherit from an anatomically calibrated coordinate frame whose scale and orientation can be easily matched to subjects using anatomical landmarks such as Lambda and Bregma for rodents. 4. Skull meshes can be loaded to aid probe implantation planning and be accounted in k-Wave acoustic simulations. Craniotomies can also be simulated with support for boolean operation. More generally, a broad variety of mesh operations can be achieved thanks to the integration of the trimesh Python library (Dawson-Haggerty, 2019). 5. Axisymmetric simulations in homogeneous domains and 3D simulations in complex mediums derived from mesh objects can be conducted in built-in Armatures. This integration alleviates the need to redefine sources and domains in external software. Quantitative assessment of the targeting of FUS stimulations can be performed programmatically by evaluating for example the intersection of the simulated FUS focal spot with a specific brain structure.

## Software architecture

The software is composed of a viewer graphical interface based on PyQt6, hosting a pyqtgraph 3D viewport. Modules are integrated to the GUI as dockable elements and allow the manipulation of objects that can be visualized in the viewport. At its core, CoperniFUS 0.1.2 is equipped with three built-in modules: 1. the Tooltip module, which allows the user to input coordinates, visualized in the viewer by an axis triad. Section views of items displayed in the viewport can be performed along planes normal to its  $x$ ,  $y$  and  $z$  axes. Furthermore, Tooltip coordinates can be referenced by any modules, facilitating anatomical landmark registration, or assessment of distances and locations in any coordinate frames. 2. The Stereotaxic

frame module handles the creation of arbitrary stereotaxic frames using armatures objects that can be combined in a hierarchical structure. At its core, an armature consists of a series of affine transformation operations (translation & rotation) that allow for the modeling of rigid frames. Specialized armature objects also exist to perform operations in the coordinates of stereotaxic frame elements. Thus, trimesh armatures have been developed to perform import .stl meshes, create arbitrary geometries programmatically or perform operations such as booleans or convexhull mesh generation. A dedicated armature object leveraging the [Python implementation of k-Wave](#) (Yagubbbayli et al., 2024) has been designed to evaluate pressure field in the context of FUS neurostimulation studies. From a programmer perspective, specialized armatures inherit from a common Armature class, which implements the coordinate transformation logic and user interface aspects. 3. Finally, the Anatomical registration helper module handles spatial transformations required to match the location, rotation and scale of atlases and objects such as skull meshes or reference images to anatomical landmarks acquired experimentally. As represented on [Figure 2](#), coordinate frame associated to modules and armatures used throughout the software are part of a common hierarchical system. Any objects displayed in the viewer can thus be easily set to inherit from the anatomically calibrated coordinate system.

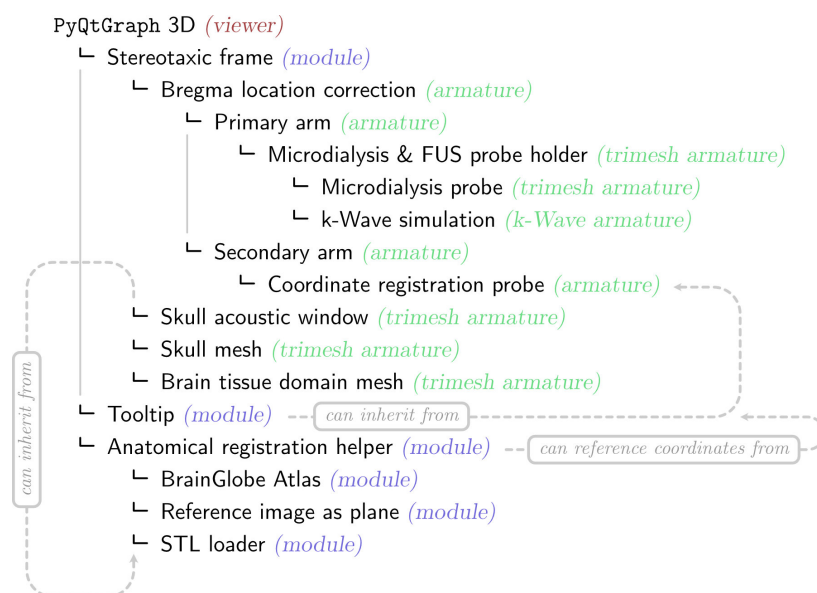

**Figure 2:** Illustration of CoperniFUS's hierarchical coordinate system in the context of a study involving ultrasound neurostimulation coupled to microdialysis sampling. From the user's perspective, this hierarchical structure of armatures can be established and edited graphically through *drag-and-drop* actions within the tree view of the Stereotaxic Frame module. Inheritance to the anatomically calibrated coordinate frame can be disabled for specific objects by setting `ignore_anatomical_landmarks_calibration` to `True` in its associated configuration dictionary.

Optional modules are also available to add brain atlases to the viewport available via the BrainGlobe API (Brain Atlas module), reference images can also be imported (Images as planes modules) as well as stl meshes (STL handler module).

Application states are continuously stored in a user readable dictionary-like json file. Multiple configuration files can be created switched between, allowing the user to save stereotaxic frame configurations and atlas anatomical registrations corresponding to specific subjects for post processing of experiments results. Configuration dictionaries for armature objects can additionally be modified in a built-in text editor. Variables contained in this dictionary can be made editable from the GUI itself, in a dedicated section of the stereotaxic frame module dock.

Finally, data analysis and manipulation can be greatly simplified by using CoperniFUS in interactive mode. The application can indeed be launched as a standalone software from a terminal, or in an interactive [Jupyter notebook](#) environment. In this mode, data manipulated in the viewer, modules and armatures can be programmatically grabbed and processed externally using Python.

## Acknowledgements

This project was supported by the French National Research Agency (ANR-16-TERC0017, ANR-21-CE19-0007 & ANR-21-CE19-0030), the American Focused Ultrasound Foundation (LabTAU, FUSF Center of Excellence). Additionally, this work was performed within the framework of the LABEX DEV WECAN (ANR-10-LABX-0061) and CORTEX (ANR-11-LABX-0042) of Université de Lyon, within the program “Investissements d’Avenir” (ANR-11-IDEX-0007) operated by the French National Research Agency (ANR). The work of the communities behind [k-Wave](#) and the Python packages used throughout this work was integral to its completion. Finally, the authors warmly thank Dr. Sandrine Parrot (CRNL, Lyon) for her strong expertise in microdialysis devices and in vivo experiments.

## References

- Aubry, J.-F., Bates, O., Boehm, C., Butts Pauly, K., Christensen, D., Cueto, C., Gélât, P., Guasch, L., Jaros, J., Jing, Y., Jones, R., Li, N., Marty, P., Montanaro, H., Neufeld, E., Pichardo, S., Pinton, G., Pulkkinen, A., Stanzola, A., ... Van 'T Wout, E. (2022). Benchmark problems for transcranial ultrasound simulation: Intercomparison of compressional wave models. *The Journal of the Acoustical Society of America*, 152(2), 1003–1019. <https://doi.org/10.1121/10.0013426>
- Aubry, J.-F., Tanter, M., Pernot, M., Thomas, J.-L., & Fink, M. (2003). Experimental demonstration of noninvasive transskull adaptive focusing based on prior computed tomography scans. *The Journal of the Acoustical Society of America*, 113(1), 84–93. <https://doi.org/10.1121/1.1529663>
- Claudi, F., Petrucco, L., Tyson, A., Branco, T., Margrie, T., & Portugues, R. (2020). BrainGlobe Atlas API: A common interface for neuroanatomical atlases. *Journal of Open Source Software*, 5(54), 2668. <https://doi.org/10.21105/joss.02668>
- Constans, C., Mateo, P., Tanter, M., & Aubry, J.-F. (2018). Potential impact of thermal effects during ultrasonic neurostimulation: Retrospective numerical estimation of temperature elevation in seven rodent setups. *Physics in Medicine & Biology*, 63(2), 025003. <https://doi.org/10.1088/1361-6560/aaa15c>
- Dawson-Haggerty. (2019). *Trimesh*.
- Dyke, K., Pépés, S. E., Chen, C., Kim, S., Sigurdsson, H. P., Draper, A., Husain, M., Nachev, P., Gowland, P. A., Morris, P. G., & Jackson, S. R. (2017). Comparing GABA-dependent physiological measures of inhibition with proton magnetic resonance spectroscopy measurement of GABA using ultra-high-field MRI. *NeuroImage*, 152, 360–370. <https://doi.org/10.1016/j.neuroimage.2017.03.011>
- Harvey, E. N. (1929). The effect of high frequency sound waves on heart muscle and other irritable tissues. *American Journal of Physiology-Legacy Content*, 91(1), 284–290. <https://doi.org/10.1152/ajplegacy.1929.91.1.284>
- Kleven, H., Bjerke, I. E., Clascá, F., Groenewegen, H. J., Bjaalie, J. G., & Leergaard, T. B. (2023). Waxholm Space atlas of the rat brain: A 3D atlas supporting data analysis and integration. *Nature Methods*, 20(11), 1822–1829. <https://doi.org/10.1038/s41592-023-02034-3>



- Min, B.-K., Yang, P. S., Bohlke, M., Park, S., R.Vago, D., Maher, T. J., & Yoo, S.-S. (2011). Focused ultrasound modulates the level of cortical neurotransmitters: Potential as a new functional brain mapping technique. *International Journal of Imaging Systems and Technology*, 21(2), 232–240. <https://doi.org/10.1002/ima.20284>
- Muller, E., Bednar, J. A., Diesmann, M., Gewaltig, M.-O., Hines, M., & Davison, A. P. (2015). Python in neuroscience. *Frontiers in Neuroinformatics*, 9. <https://doi.org/10.3389/fninf.2015.00011>
- Murphy, K. R., Farrell, J. S., Bendig, J., Mitra, A., Luff, C., Stelzer, I. A., Yamaguchi, H., Angelakos, C. C., Choi, M., Bian, W., Dilanni, T., Pujol, E. M., Matosevich, N., Airan, R., Gaudillière, B., Konofagou, E. E., Butts-Pauly, K., Soltesz, I., & De Lecea, L. (2024). Optimized ultrasound neuromodulation for non-invasive control of behavior and physiology. *Neuron*, S0896627324004938. <https://doi.org/10.1016/j.neuron.2024.07.002>
- Murphy, K. R., Nandi, T., Kop, B., Osada, T., Lueckel, M., N'Djin, W. A., Caulfield, K. A., Fomenko, A., Siebner, H. R., Ugawa, Y., Verhagen, L., Bestmann, S., Martin, E., Pauly, K. B., Fouragnan, E., & Bergmann, T. O. (2025). A practical guide to transcranial ultrasonic stimulation from the IFCN-endorsed ITRUSST consortium. *Clinical Neurophysiology*, S1388245725000148. <https://doi.org/10.1016/j.clinph.2025.01.004>
- Olaitan, G. O., Ganesana, M., Strohmman, A., Lynch, W. J., Legon, W., & Jill Venton, B. (2024). *Focused Ultrasound Modulates Dopamine in a Mesolimbic Reward Circuit*. <https://doi.org/10.1101/2024.02.13.580202>
- Pichardo, S. (2023). BabelBrain: An Open-Source Application for Prospective Modeling of Transcranial Focused Ultrasound for Neuromodulation Applications. *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, 70(7), 587–599. <https://doi.org/10.1109/TUFFC.2023.3274046>
- Sammartino, F., Beam, D. W., Snell, J., & Krishna, V. (2020). Kranion, an open-source environment for planning transcranial focused ultrasound surgery: Technical note. *Journal of Neurosurgery*, 132(4), 1249–1255. <https://doi.org/10.3171/2018.11.JNS181995>
- Suarez-Castellanos, I. M., Dossi, E., Vion-Bailly, J., Salette, L., Chapelon, J.-Y., Carpentier, A., Huberfeld, G., & N'Djin, W. A. (2021). Spatio-temporal characterization of causal electrophysiological activity stimulated by single pulse focused ultrasound: An ex vivo study on hippocampal brain slices. *Journal of Neural Engineering*, 18(2), 026022. <https://doi.org/10.1088/1741-2552/abdfb1>
- Treeby, B. E., & Cox, B. T. (2010). K-Wave: MATLAB toolbox for the simulation and reconstruction of photoacoustic wave fields. *Journal of Biomedical Optics*, 15(2), 021314. <https://doi.org/10.1117/1.3360308>
- Verhagen, L., Gallea, C., Folloni, D., Constans, C., Jensen, D. E., Ahnine, H., Roumazeilles, L., Santin, M., Ahmed, B., Lehericy, S., Klein-Flügge, M. C., Krug, K., Mars, R. B., Rushworth, M. F., Pouget, P., Aubry, J.-F., & Sallet, J. (2019). Offline impact of transcranial focused ultrasound on cortical activation in primates. *eLife*, 8, e40541. <https://doi.org/10.7554/eLife.40541>
- Wang, Q., Ding, S.-L., Li, Y., Royall, J., Feng, D., Lesnar, P., Graddis, N., Naeemi, M., Facer, B., Ho, A., Dolbeare, T., Blanchard, B., Dee, N., Wakeman, W., Hirokawa, K. E., Szafer, A., Sunkin, S. M., Oh, S. W., Bernard, A., ... Ng, L. (2020). The Allen Mouse Brain Common Coordinate Framework: A 3D Reference Atlas. *Cell*, 181(4), 936–953.e20. <https://doi.org/10.1016/j.cell.2020.04.007>
- Yaakub, S. N., White, T. A., Roberts, J., Martin, E., Verhagen, L., Stagg, C. J., Hall, S., & Fouragnan, E. F. (2023). Transcranial focused ultrasound-mediated neurochemical and functional connectivity changes in deep cortical regions in humans. *Nature Communications*, 14(1), 5318. <https://doi.org/10.1038/s41467-023-40998-0>

Yagubbbayli, Farid and Sinden, David and Simson, & Walter. (2024). *K-Wave-Python*.

Yang, P. S., Kim, H., Lee, W., Bohlke, M., Park, S., Maher, T. J., & Yoo, S.-S. (2012). Transcranial Focused Ultrasound to the Thalamus Is Associated with Reduced Extracellular GABA Levels in Rats. *Neuropsychobiology*, 65(3), 153–160. <https://doi.org/10.1159/000336001>